


MAR 21 2011

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130187 ✓
Name	Dan Pasquariello	ID#	2620 ✓
		Date	3-15-11 ✓
A	Agency	Dillingham PD	Phone # 842-5354
	Instrument Location	Dillingham PD	
B	Alco S/N	70108 ✓ <del>70180</del> DWN	Target Value .081 ✓
			High Pressure 700 psi
	Alco Test Values	.082 ✓ 1st Alco	.082 ✓ 2nd Alco
	Signature		
(OVER)			


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

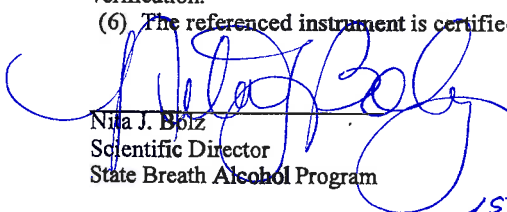  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 1<sup>ST</sup> day of APRIL, 2011 DWN

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

100187 BMB  
3/31/11

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

MARCH 15, 2011

OPERATOR'S NAME:

PASQUARIELLO, DAN

OPERATOR'S NUMBER: 2620

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/NI :

UOC

O.L. #: 1234567890

DEPT/AGENCY: DL61

CASE/REPORT: 1234567890

TEST TYPE: U

ALCO TARGET VALUE: .001

ALCO S/N: 70100

### — BREATH ANALYSIS —

.001 ADJUSTED FOR 29.52 in		
ALCO TARGET	.079	09:46
BLANK TEST	.000	09:47
INTERNAL STANDARD	VERIFIED	09:47
ALCO TV 29.52 in	.002	09:47
BLANK TEST	.000	09:48
SUBJECT SAMPLE	.000	09:49
BLANK TEST	.000	09:50
ALCO TV 29.52 in	.002	09:50
BLANK TEST	.000	09:51

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130187

MARCH 15, 2011

TIME 09:52

### — DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.52 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

! " # % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢